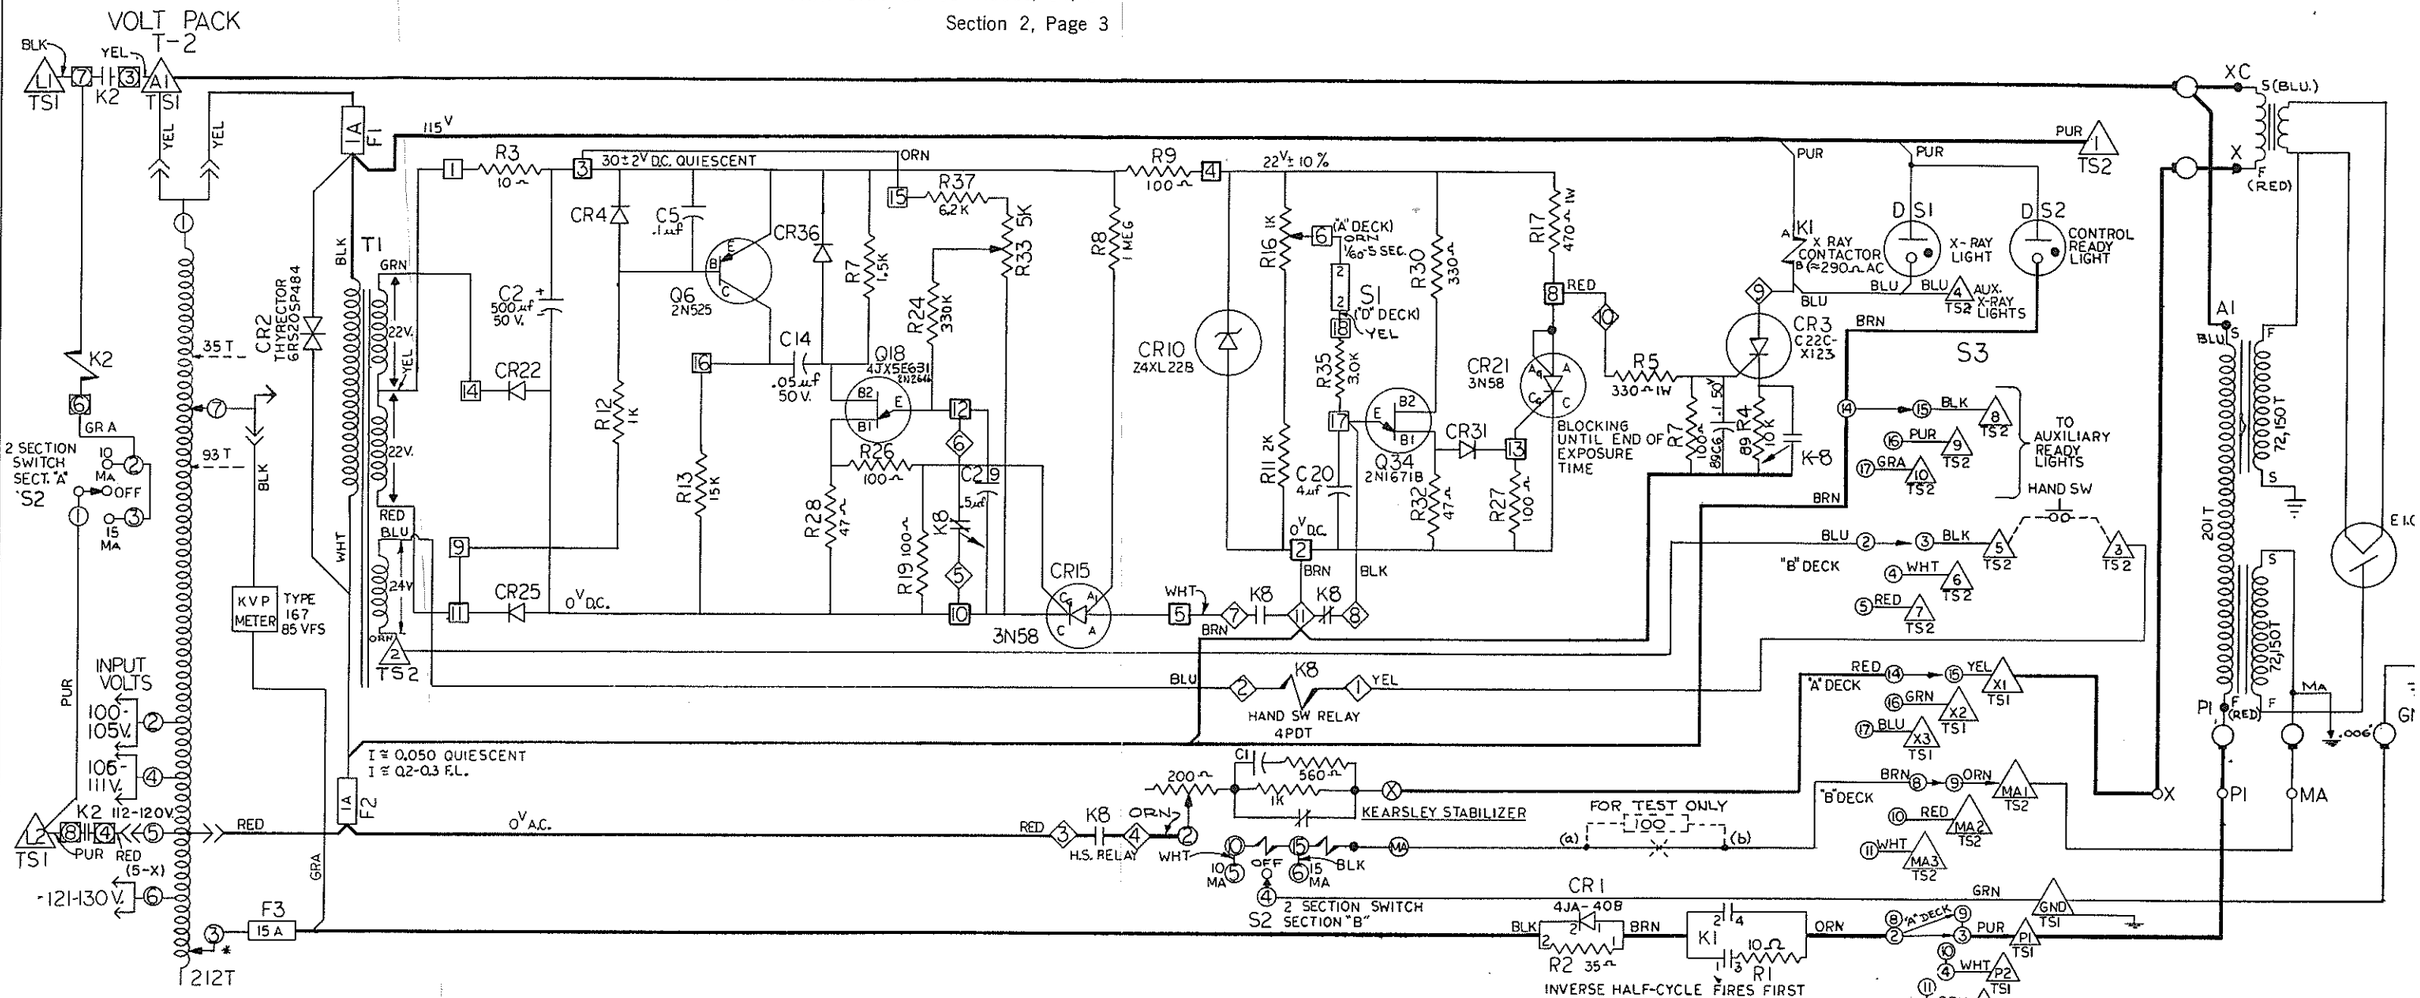

* - CALIBRATION DATA - 5% LINE OR BETTER

10 MA		15 MA	
KVP	PRIM. LOAD VOLTS	KVP	PRIM. LOAD VOLTS
50	58.5	50	63
60	68	60	72.5
70	78	70	82
80	87.5	80	91
90	97	90	100.5
100	106.5		

NOTES:
1. ALL RESISTORS ARE ½ W., 5% UNLESS OTHERWISE SPECIFIED.
2. ALL CAPACITORS ARE 100 V., UNLESS OTHERWISE SPECIFIED.

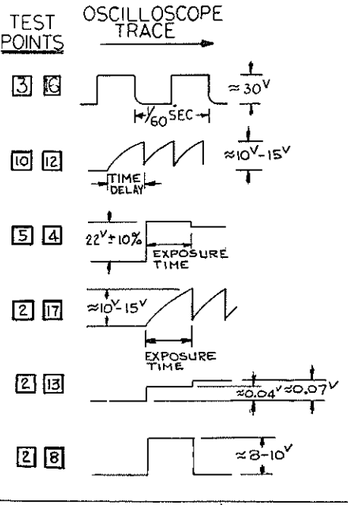

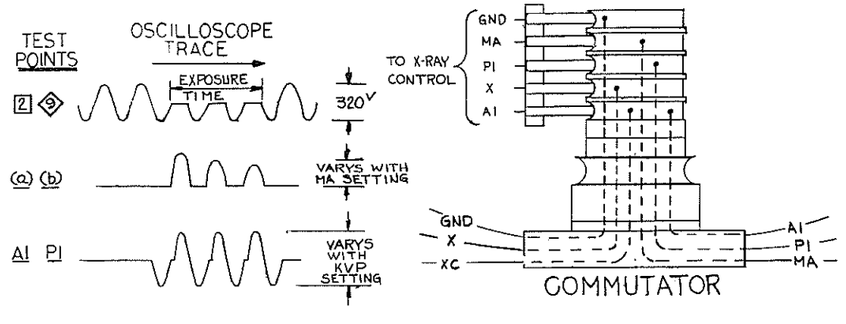

SI TIMING HEAD
(ALL VALUES IN KILOHMS)

TIMER SETTING	NOMINAL RESIST	TIMER SETTING	NOMINAL RESIST	TIMER SETTING	NOMINAL RESIST
1/60	0	12/60	43.57	1	238.6
2/60	3.83	15/60	55.33	1-1/4	301
3/60	7.87	18/60	68.1	1-1/2	360.37
4/60	11.70	21/60	79.8	1-3/4	420.6
5/60	15.8	24/60	91.8	2	483.53
6/60	19.63	30/60	115.5	3	715
8/60	27.50	36/60	143	4	961.8
10/60	35.7	48/60	190.4	5	1202.57

SCHEMATIC DIAGRAM

GE - 100 REMOTE TYPE

(CONTROL MODEL 11CE8A1, TUBE HEAD MODEL 11AA5A1)

9449-D40